



Test Equipment  
Depot  
1-800-517-8431

## User Guide

99 Washington Street  
Melrose, MA 02176  
Phone 781-665-1400  
Toll Free 1-800-517-8431



Visit us at [www.TestEquipmentDepot.com](http://www.TestEquipmentDepot.com)

# EasyView Digital Light Meter

## Model EA31



## **Introduction**

Thank you for selecting the Extech EasyView Digital Light Meter which measures the amount of light falling on a surface (luminance) in Foot-candles or Lux. This device measures up to 20,000 Fc and 20,000 Lux. This device is shipped fully tested and calibrated and, with proper use, will provide years of reliable service.


## **Meter Description**

1. LCD display
2. Range button
3. Power ON/OFF button
4. lux / fc selection button
5. Data HOLD button
6. MAX/MIN button
7. Photo sensor (lens cover not shown)  
(Tripod mounts on rear of sensor)

Note: Battery compartment is located  
on the rear of the instrument



## **Spectral Sensitivity**

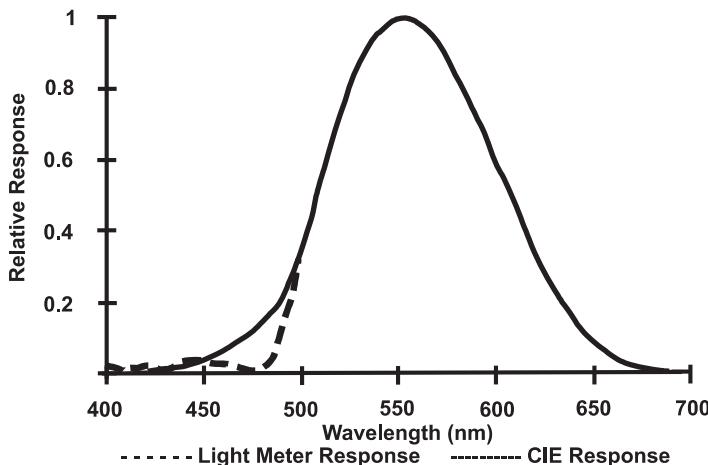

## **Operation**

---

### **Power ON or OFF**

Press the  button to turn power on or off.

### **Units of measure**

Press the lux / fc button to select the unit of measure. "fc" or "lux" will appear in the display.

### **Light sensor**

1. The light sensor is attached to the meter with a coiled cable which allows placement of the sensor up to approximately 3 feet from the meter.
2. The light sensor is a silicon photo diode and resides under the white domed lens.
3. To protect the lens from scratches, keep the protective cap on the sensor whenever the unit is not in use.
4. The back of the sensor has a tripod mounting hole.

### **Taking measurements**

1. Remove the protective cap from the sensor.
2. Place the sensor in a horizontal position at the measurement location.
3. Read the light level on the display. If the light measurement is out of range an "OL" indication will appear on the display. If the 'OL' appears, select a higher range by pressing the RANGE button.

### **MX MN Function**

1. Press the MX/MN button once to put the meter in MX/MN mode. The meter will now display the highest reading that occurs while the function is enabled. The "**MAX**" icon will appear in the display.
2. Press the MX/MN button again to display the lowest reading that occurs while the function is enabled. The "**MIN**" icon will appear in the display.
3. Press MX/MN again to toggle between the MAX and MIN readings.
4. To exit the MX MN mode and return to the normal real time display, press and hold the MX/MN button (2 seconds) until the **MAX** and **MIN** icons disappear.

### **Data Hold**

Press the **HOLD** button to freeze the displayed reading. The  hold icon will appear on the display. Press the **HOLD** button again to return to normal operation.

## **Reference**

---

<b>Foot candles</b>	<b>Lux</b>	<b>Typical Light Levels</b>
>10000	>107600	Sunlight
1000 to 10000	10760 to 107600	Operating Table
100 to 1000	1076 to 10760	Assembly (fine) Football stadium Emergency room Drafting table
10 to 100	107 to 1076	Overcast day Assembly (general) Classroom Casual reading Shipping area Stairwell Auditorium
1 to 10	10.7 to 107	ATM machine Storage room Building entrance Parking lot
0 to 1	0 to 10.7	Highway Full moon

### **Foot-candle / Lux conversion**

1 lux = .09290 foot-candles

1 foot-candle = 10.764 lux

## Maintenance

---

### Cleaning and storage

1. The white plastic sensor dome should be cleaned with a damp cloth when necessary.
2. Store the meter in an area with moderate temperature and humidity (refer to the operating and storage range in the specifications chart earlier in this manual).

### Battery Replacement

When the battery voltage is low the 'BT' symbol will appear on the display. Replace the six (6) 1.5 'AAA' batteries by removing the rear (center) battery compartment screw and accessing the battery compartment. Observe polarity when placing the batteries in the compartment. Ensure that the compartment cover is securely fastened when finished.



You, as the end user, are legally bound (**Battery ordinance**) to return all used batteries and accumulators; **disposal in the household garbage is prohibited!**  
You can hand over your used batteries / accumulators at collection points in your community or wherever batteries / accumulators are sold!

**Disposal:** Follow the valid legal stipulations in respect of the disposal of the device at the end of its lifecycle

## Specifications

---

Ranges	Resolution	Accuracy
<b>Lux</b>		
20.00, 200.0 2000	0.01 0.1 1	± (3% Reading + 0.5% Full Scale)
20.00kLux	0.01	if > 10,000 lux ±( 4% Reading + 0.5%Full Scale)
<b>Foot candles</b>		
20.00 200	0.01 0.1	± (3% Reading + 0.5% Full Scale)
2000, 20.00kfc	1 0.01	if > 1,000 fc ±( 4% Reading + 0.5%Full Scale)

## **General Specifications**

Display	3-1/2 digit, 2000 count LCD
Over range indication	LCD displays 'OL'
Spectral response	CIE photopic (CIE human eye response curve), Cosine corrected
Spectral accuracy	CIE V <sup>2</sup> function ( $f_1, 6\%$ )
Measurement Repeatability	$\pm 2\%$
Calibration	Calibrated to a standard incandescent lamp at color temperature 2856°K
Temperature coefficient	$\pm 0.1\%$ per °C
Sampling rate	2.5 times per second
Photo detector	Silicon photo-diode and spectral response filter
Operating conditions	Temperature: 0 to 40°C (32 to 104°); Humidity: < 80% RH
Storage conditions	Temperature: -10 to 50°C (14 to 140°F); Humidity: < 80% RH
Dimensions	150 x 72 x 35mm (5.91 x 2.8 x 1.4")
Weight	Approx. 320g (11.3 oz) with battery
Photo Detector Dimensions	92 x 60 x 29mm (3.62 x 2.36 x 1.14")
Detector cable length	91cm (3') approximately
Low battery indication	"BT" appears on the LCD
Power supply	6 'AAA' cells; Battery life approx 400 hours

**Copyright © 2013 FLIR Systems, Inc.**

All rights reserved including the right of reproduction in whole or in part in any form  
**ISO-9001 Certified**